


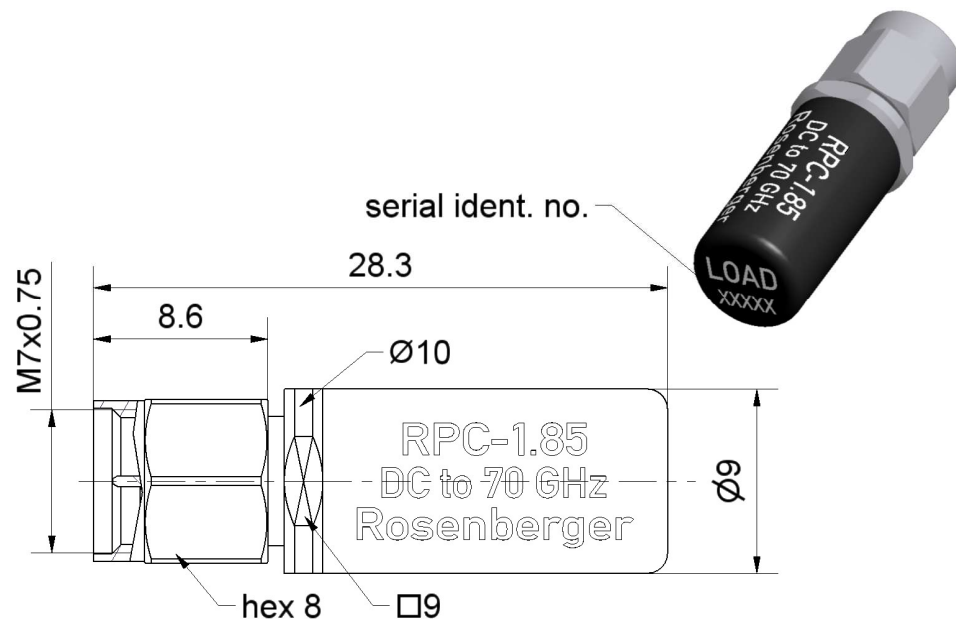

All dimensions are in mm; tolerances according to ISO 2768 m-H

Interface

According to
Mechanically compatible with

IEC 61169-32
RPC-2.40

Documents

Application note

AN001 "Calibration Services"

Material and plating

Connector parts

Center contact
Outer contact
Coupling nut
Dielectric
Substrate

Material

Beryllium copper
Stainless steel
Stainless steel
PS
Al₂O₃

Plating

Gold, min. 1.27 µm, over nickel
Passivated
Passivated

Electrical data

Frequency range	DC to 70 GHz
Return loss	≥ 35 dB, DC to 4 GHz ≥ 26 dB, 4 GHz to 40 GHz ≥ 22 dB, 40 GHz to 70 GHz
DC Resistance	$50\ \Omega \pm 0.25\ \Omega$
Power handling	≤ 0.5 W

Mechanical data

Mating cycles	≥ 500
Maximum torque	1.65 Nm
Recommended torque	0.90 Nm
Gauge	0.00 mm to 0.03 mm

General standard definitions

For proper operation the vector network analyzer (VNA) needs a model describing the electrical behaviour of this calibration standard. The different models, units, and terms used will depend on the VNA type and they will have to be entered into the VNA. All values are based on typical geometry and plating.

Offset Z_0 / Impedance / Z_0	50 Ω
Offset Delay	0.0000 ps
Length (electrical) / Offset Length	0.000 mm
Offset Loss	0.00 G Ω /s
Loss	0.0000 dB/ $\sqrt{\text{GHz}}$

Environmental data

Operating temperature range ¹	+20 °C to +26 °C
Rated temperature range of use ²	0 °C to +50 °C
Storage temperature range	- 40 °C to +85 °C

RoHS compliant

¹ Temperature range over which these specification are valid.

² This range is underneath and above the operating temperature range, within the calibration load is fully functional and could be used without damage.

Technical Data Sheet		Rosenberger							
RPC-1.85	Calibration Load Plug	08S150-C10S3							
Declaration of calibration options Factory Calibration Standard delivery for this calibration standard includes a Factory Calibration. The Calibration Certificate issued reports individual calibration results, traceable to national / international standards. Model based standard definitions are reported in an Agilent/Keysight, Rohde & Schwarz and Anritsu compatible VNA format. Accredited Calibration Not available. For further, more detailed information see application note AN001 on the Rosenberger homepage. Calibration interval <table><tr><td>Recommendation</td><td>12 months</td></tr></table> Packing <table><tr><td>Standard</td><td>1 pce in box</td></tr><tr><td>Weight</td><td>6.8 g/pce</td></tr></table>				Recommendation	12 months	Standard	1 pce in box	Weight	6.8 g/pce
Recommendation	12 months								
Standard	1 pce in box								
Weight	6.8 g/pce								
While the information has been carefully compiled to the best of our knowledge, nothing is intended as representation or warranty on our part and no statement herein shall be construed as recommendation to infringe existing patents. In the effort to improve our products, we reserve the right to make changes judged to be necessary.									
Draft	Date	Approved	Date	Rev.	Engineering change number	Name	Date		
Kerstin Herzog	26.09.05	Lars Ramtke	21.01.21	f00	20-2460	Marion Striegler	21.01.21		
Rosenberger Hochfrequenztechnik GmbH & Co. KG P.O.Box 1260 D-84526 Tittmoning Germany www.rosenberger.de				Tel. : +49 8684 18-0 Email : info@rosenberger.de			Page 3 / 3		